

# Frequency Dependent Planar Electromagnetic Modeling of Human Body and Theoretical Study on Attenuation for Power Budget Estimation of UWB Radar

Kedar Nath Sahu<sup>1</sup> and Dr. Challa Dhanunjay Naidu<sup>2</sup>

<sup>1</sup> Stanley College of Engineering and Technology for Women, Chapel Road, Abids, Hyderabad, Andhra Pradesh

*Received: 12 December 2013 Accepted: 5 January 2014 Published: 15 January 2014*

---

## Abstract

Detection of the heartbeat rate and/or respiration rate are very important for most radar based applications like lie-detection, life-detection etc. The prediction of signal losses is a fundamental aspect in the design of ultra wide-band radars. The effect of body tissues surrounding the heart is important in the design of a radar system used for heartbeat detection. The broad variety of tissues and their frequency dependent behavior makes accurate attenuation prediction very difficult without the support of an appropriate model. In this paper, two frequency dependent planar electromagnetic models viz. intrinsic impedance model (a classical model) and impedance transformation model, both incorporating dispersive dielectric properties are discussed. Signal attenuations in both models are estimated and compared. This estimation can be helpful in the design of an ultra wideband (UWB) radar system meant for cardio-pulmonary activity related applications.

---

**Index terms**— ultra wideband (uwb), radar, modeling, signal attenuation, reflection coefficient, power budget etc.

## 1 Introduction

or many applications such as lie detection, life detection etc. remote detection/monitoring of cardio-pulmonary features of a human being such as heartbeat rate, breath rate, and blood flow rate etc. are necessary. This can be done to good accuracy using high resolution radars like ultra wide-band radars. Moreover, human body monitoring using UWB technology can permit the subject to be in absolutely free space as it uses radiated field unlike other methods e.g. functional-MRI (f-MRI) uses induced EM field. A summary of the existing models found in the literature are presented below.

Radar monitoring of human physiologic functions started in early 70's as mentioned in [1] but further progress was stopped as the technique was expensive. Micro-power Impulse Radar (MIR), an UWB radar model was developed by Thomas E. McEwan at Lawrence Livermore National Laboratory (LLNL) during 1993 which was able to detect the movements of heart wall from the difference of reflection magnitude between various tissue interfaces. This model proposed in both of the patents on medical UWB radar awarded to McEwan [2][3], did not account for the various living tissues through which the UWB pulse travels before it strikes the heart wall and hence is quite ingenuous. Another more accurate model described in [4] was found at Tor Vergata University of Rome, Italy that accounted for thickness, impedance, linear attenuation and wave velocity of six superimposed living tissues (air, fat, muscle, cartilage, deflated lung and heart) encountered by the UWB pulse passing through the chest from skin to heart. This model was based on the data taken from Visible Human Project [5] and Gabriel's data book of dielectric properties of tissues [6]. As an immediate application of this model the author of this model [4] developed the UWB radar based stealthy lie detector [7]. The attenuation predicted by the

model given in [4] was linear but the imaginary part of reflection coefficient and multiple reflections were ignored. In [4], author himself mentioned that this new model remains intrinsically wrong as the dielectric properties used were measured on living tissues using a continuous-wave (CW) of frequency 1500 MHz. The analysis was based on only one frequency and therefore was frequency independent. Hence the author suggested for a more effective model by using ultra wide-band dielectric properties instead of narrow band ones for which a convolution method or a Finite Difference Time Domain (FDTD) technique should be used and also by considering both the real and imaginary parts of the reflection coefficients at the boundaries because the UWB receiving correlator, working in the time domain, is strongly sensitive to phase errors. [8] which could predict the response of a four layer biological model with three layers of normal tissue and one layer of cancerous soft tissue to input UWB signal. The thickness of each layer in the models was taken from the Visible Human Project [5] and dielectric properties of tissues from Gabriel's data book [6] as followed by the earlier model presented in [4]. As far as the planar technique is concerned the authors mentioned that the technique produces reasonable results for applications of less number of layers but not very accurate for more complex layers as it does not consider to model multiple reflections and hence suggested that the planar technique could be extended to include provision for multiple reflections.

A circuitual model for monitoring of cardiopulmonary activity with UWB radar of operating frequency range of 0.1 to 3 GHz was presented in 2008 by Pisa et.al [9]. This model was developed taking the signal source, transmitting and receiving antenna properties as well as a planar model of human thorax into account. The thorax model considered the same tissues: air, fat, muscle, cartilage, lung and heart as used in the model employed in [4]. The attenuation of the air-heart-air path was evaluated over the ultra wideband frequency of 0.1 to 3 GHz for two types of lungs: deflated lung and inflated lung. It was found that the model has predicted attenuation increase with frequency and moreover the amount of attenuation increase is more in case of deflated lung than that in case of inflated lung [9]. This planar model was a circuitual model but, an electromagnetic (EM) model could be a more approximate model over circuitual model.

Both the UWB models reported in [4] and [9] ignored the skin tissue in the thoracic modeling but attenuation due to skin tissue is also significant because skin is also one of the greatest electromagnetic field absorbing tissues like muscle and blood in the human body as reported in [10]. Moreover, the circuitual model given in [9] is frequency dependent whereas the model described in [4] was developed for a continuous wave of 1.5 GHz and hence was a frequency independent model. A frequency dependent planar model described in [8] considers skin but did not include the phenomenon of multiple reflections.

Also, calculations pertaining to incident, reflection and transmission components of power at every interface are considered, which are not calculated and reported by any of the models. An investigation of these effects such as accounting for the electromagnetic information due to skin, the phenomenon of multiple reflections, frequency dependence of signal attenuation is the subject of this paper.

In this paper, two frequency-dependent planar electromagnetic models of human thorax: the intrinsic impedance or classical model and the impedance transformation model are reported in which both models incorporate the dispersive behavior of selected biological tissues including skin. When the impedance transformation model takes care of the effect of multiple reflections, the classical model does not consider that effect. First, without including skin in the modeling, the signal attenuation results are obtained and compared with the attenuation results reported in the circuitual model of [9]. Then the signal attenuation results from the heart with skin included in both the models are analyzed and compared.

As skin tissue is included in the thoracic modeling and particularly, the multiple reflections are also taken care of by the impedance transformation model the signal attenuation results predicted by the models presented in this paper are considered to be more realistic than the model-predicted attenuation of the circuitual model reported in [9].

## 2 II.

### 3 Theoretical Background

In order to study the behavior of the backscattered field from a human body illuminated by plane electromagnetic waves of a radar transmitter, simplification of the problem is considered by modeling the human body as a series of biological tissue layers of complex impedances. Knowing the dielectric properties of the biological tissues, and by utilizing the basic principles of electromagnetic wave propagation in accordance with the physical processes that determine the speed of propagation and the amount of attenuation, the power received by the radar receiver, the electric field (E-field) reflection coefficients at every interface and power reflection coefficient of the heart can be determined. In order to model the electromagnetic response of human body to radar waves, it is necessary to know with sufficient precision the electromagnetic characteristics of typical biological tissues used to build the body. For this purpose, the transverse section of human anatomy taken from web [11] as shown in Fig. ?? is referred. The figure depicts the human thorax showing the contents of the middle and the posterior mediastinum. The pleural and pericardial cavities are exaggerated since normally there is no space between parietal and visceral pleura and between pericardium and heart. Various tissues like sternum, hard cholesterol, muscle, ribs, costal pleura, pleural cavity, pulmonary pleura, pericardium cavity, heart, pulmonary artery (left and right), aorta, internal mammary vessels, thoracic aorta, esophagus, bronchus, thoracic duct, body of thoracic vertebrae, lungs

(left and right) etc. encounter in the path of propagation partly or fully, when the human body is illuminated by the radar wave. Let us consider only some of the major biological tissues such The anatomical thickness values of the tissue layers (Table 1) considered in both of the models are based on the Visible Human Project [5] like those already employed in the UWB models of [4], [7][8][9][10]. Based on the Cole and Cole equation as mentioned in [9] that describes the dispersive behavior of tissues, the frequency dependent dielectric bodies of human body tissues are computed as given in the Gabriel's data book of dielectric properties of tissues [6] and are also reported on the web [13].

## 4 Global Journal of Researches in Engineering

In our work, the dielectric properties such as complex relative permittivity, conductivity, attenuation constant, phase-shift constant, complex impedance and velocity of wave propagation of the selected tissues for modeling at all frequencies of 0.1 to 3 GHz ultrawideband are taken from [6]. The variations of the above dielectric properties as a function of frequency are plotted in Fig. ?? . It is seen that as frequency increases, relative permittivity decreases, but conductivity, attenuation constant, phase-shift constant and intrinsic impedance increase as shown in Fig. ??(a) -(e) respectively.

(a) as skin, fat, muscle, cartilage, lungs (deflated and inflated separately) and heart as the fundamental layers for a simple one-dimensional modeling of human body. As electromagnetic behavior due to heartbeat movements are of interest, assuming the radiation exposure from anterior of the of the human body to the posterior through heart, the tissue structure considered in view of the electromagnetic body modeling is as shown in Fig. 2.

## 5 Electromagnetic Analysis

When an electromagnetic wave is incident on an interface between two consecutive tissue layers a part of the EM energy is transmitted and the remaining is reflected [8] as shown below in Fig. 4. The amount of reflection and transmission of energy depends on the frequency dependent dielectric properties of the layers on either side of the interface. As biological tissues are lossy media, from an electromagnetic point of view they are characterized in terms of the attenuation constant, phase-shift constant, conductivity, complex permittivity, complex impedance, complex reflection coefficient etc. These characterization parameters are highly frequency dependent. Therefore, the reflected and transmitted power at all tissue interfaces calculated at every individual frequency of the ultra wide-band range using the concept of EM wave propagation in lossy media are as described in [14].

## 6 a) Propagation in Lossy Media

Wave losses due to electric field are described through complex permittivity,  $\epsilon$ . Similarly, complex permeability,  $\mu$  is used to model the losses owing to medium response to the magnetic field.

But from wave propagation point of view in most of the materials, the magnetic response is usually very weak compared to the dielectric response. Therefore,  $\mu \approx \mu_0$  i.e.  $\mu_r \approx 1$ ,  $\mu_r'' = 0$

Consequently, wave losses can be confined to the loss due to the complex permittivity only assuming  $\mu$  entirely real for the analytical loss calculation. As in [14-15], for a lossy dielectric media  $D = \epsilon E$  (1)  $J = \sigma E$  (2)  $B = \mu H$  (3)

where  $\epsilon$ , Complex permittivity =  $\epsilon' - j\epsilon''$  and  $\mu$ , Complex permeability =  $\mu' - j\mu''$

b) Characterization of loss Considering the human tissues as homogeneous, isotropic, and dispersive media, the characterization parameters such as complex propagation constant (?), complex attenuation constant (?), complex phase-shift constant (?) and complex intrinsic impedance(??) as defined in [14-15] are given as below.

Propagation constant, (6) Now,  $\text{Re}\{\gamma\} = \alpha$ , attenuation constant (7) and  $\text{Im}\{\gamma\} = \beta$ , phaseshift constant (8) where LossTangent (9) The characteristic impedance of a medium is given by Magnitude of complex impedance, can be given by, (11) Phase of complex impedance can be given by, (13) In this way the electromagnetic propagation through a medium is modeled.

7 IV.

## 8 Power Calculations

Using the power relations given in [14-15] as a general rule for average power transfer per unit area through reflection and transmission about an interface separating two lossless dielectric regions 1 and 2, incident, reflected and transmitted power for every interface can be determined.

## 9 Incident power, (14)

Reflected power, (

Transmitted power, (16)? = ? + j? = ??? = ???(? ' -j? " ) =??? ' ?1-j? " ? ' ? =? ? ?? ' 2? ? 1+ ? ? " ? ' ? 2-1? 1 2 ? =? ? ?? ' 2 ??1+(LossTangent) 2-1? 1 2 ? = ? ? ?? ' 2 ? ? 1+ ? ? " ? ' ? 2 +1? 1 2 ? = ? ? ?? ' 2 ??1+(LossTangent) 2-1? 1 2 ? = ? " ? ' = ? ? ? ' ? |?|= ?|? ? ? | ?1+ ?? ? ?? ?? 2 ? 1 4 ? ?|?= ??? ?? ' -j? " ? ? ? ?1+?? ? ??? ' -j? " ? ?? 2 ? 1 4 ? ? ?|?= ?p 0 ? 0 ? ?|1 (? r ' -j? r " ) ? | ?1+ ?? ? ?? 0



---

attenuation results thus calculated are analyzed and compared with each other and also with the attenuation results reported by the circuital model [9] as well.

A comparison of conductivity, reflection coefficients at the lung-heart interface of both intrinsic impedance model and impedance transformation model is shown in Fig. 6. It is clear that the conductivity of both deflated lung and inflated lung increase with frequency, the reflection coefficients of both lung types decrease with frequency. Also, at any frequency, deflated lung has higher conductivity and hence lesser reflection coefficient than inflated lung. In both of the models it is found that the increase of attenuation is higher in case of deflated lung than that in case of inflated lung for both without-skin and with-skin cases. This is due to the fact that deflated lung has higher conductivity [Fig. 6(a)] and hence lesser reflection coefficient than inflated lung [Fig. 6(b)]. The amount of increase of attenuation from inflated to deflated lung at a particular frequency is the same between without-skin and its corresponding with-skin case of the same model. Such an increased attenuation characteristics from inflated to deflated lung was reported in the circuital model [9] but the models presented in this work predict more attenuation for both deflated and inflated lung cases.

## VII.

## Conclusions

Remote monitoring applications based on detection of heart and breath rates are effective because it is difficult to suppress completely the heartbeat and respiration related subjects' motions. Also, the propagation of waves through the subjects' body is mainly governed by the electromagnetic characteristics of body tissues. The electromagnetic response of the human tissue is highly frequency dependent.

In this paper, both of the frequency dependent electromagnetic models of human body presented incorporate the electromagnetic properties of body tissues including the skin tissue corresponding to a 0.1 to 3 GHz ultra wide-band (UWB) radar. The lossy power coefficients at all tissue interfaces are evaluated during both forward and backward propagations of UWB pulses. The reflection from the cardiac structure i.e. the heart wall has been quantified and a comparative analysis on attenuation due to the pulse-echo intensity is presented. The complex reflection coefficients and complex impedances of tissue layers are considered in this one-dimensional analytical solution as they are important for the validity of power budget analysis. The advantage of the planar impedance transformation model is the implicit inclusion of the electromagnetic wave phenomenon such as multiple reflections, taking place during propagation through multiple interfaces.

Owing to the inclusion of the effect of skin tissue in the planar modeling along with the implicit provision for multiple reflections, the impedance transformation model can have better prediction ability of signal attenuation in the design of UWB radars. Future work will involve the application of impedance transformation model for other biological applications for study of signal attenuation. Results of such complex and sophisticated biological models shall help to build and test signal processing techniques in non-invasive, remote monitoring applications like home health care, emergency rooms, intensive care units (ICUs) in hospitals, pediatric clinics to alert for sudden infant death syndrome (SIDS), radar based lie detection, remote life detection etc. the heartbeat signal power thus derived can be processed further to obtain heart beat information.

---

<sup>1</sup>© 2014 Global Journals Inc. (US)

<sup>2</sup>Frequency Dependent Planar Electromagnetic Modeling of Human Body and Theoretical Study on Attenuation for Power Budget Estimation of UWB Radar



Figure 1:

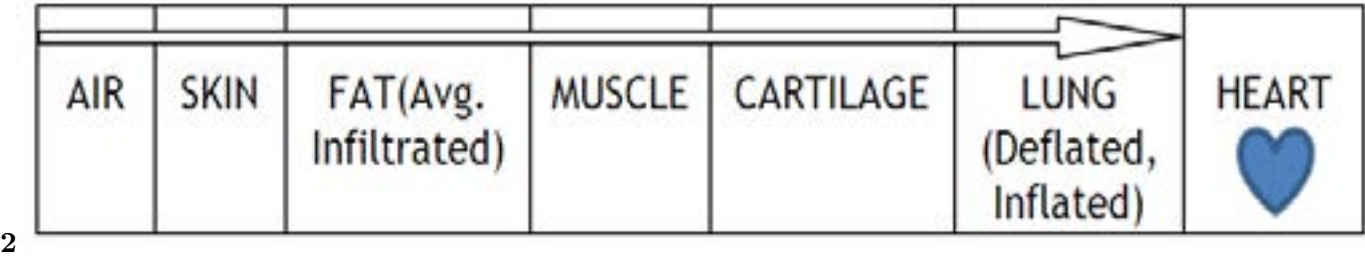


Figure 2: Figure 2 :



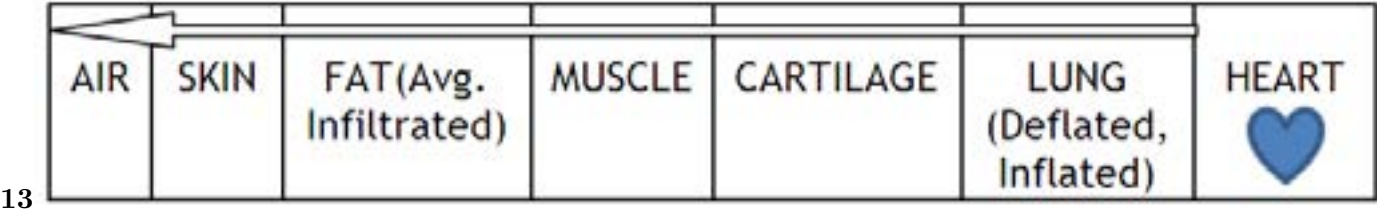


Figure 3: Figure 1 :Figure 3 :

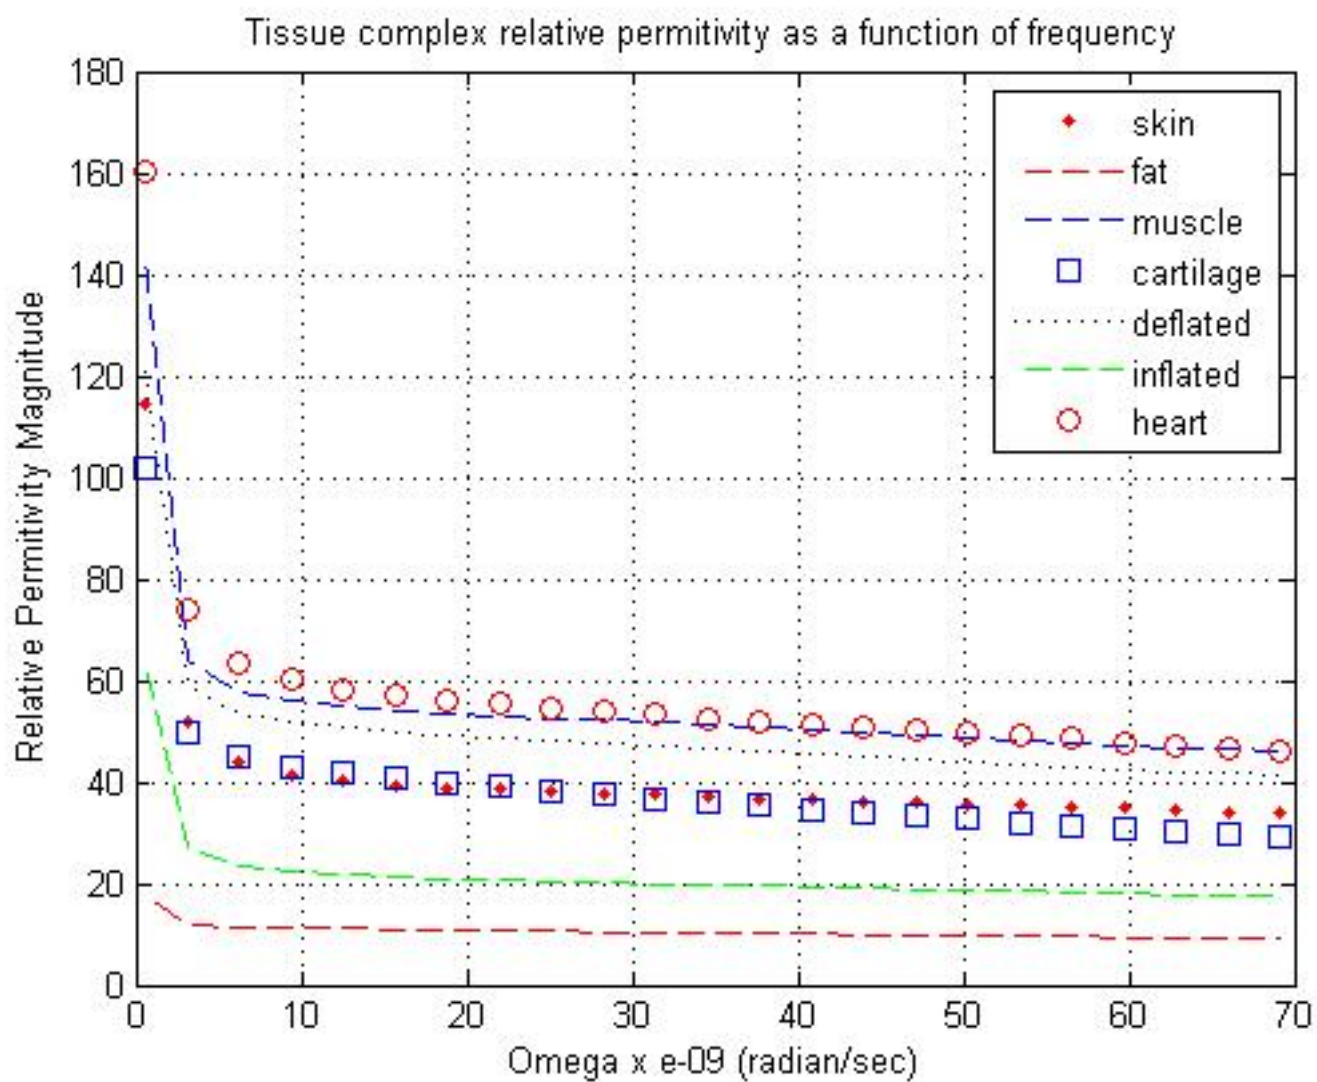

4


Figure 4: Figure 4 :

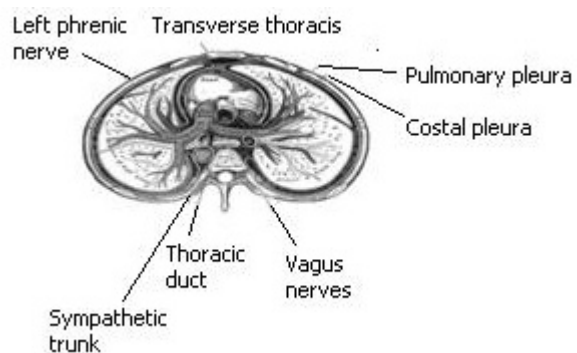

5

Figure 5: Figure 5




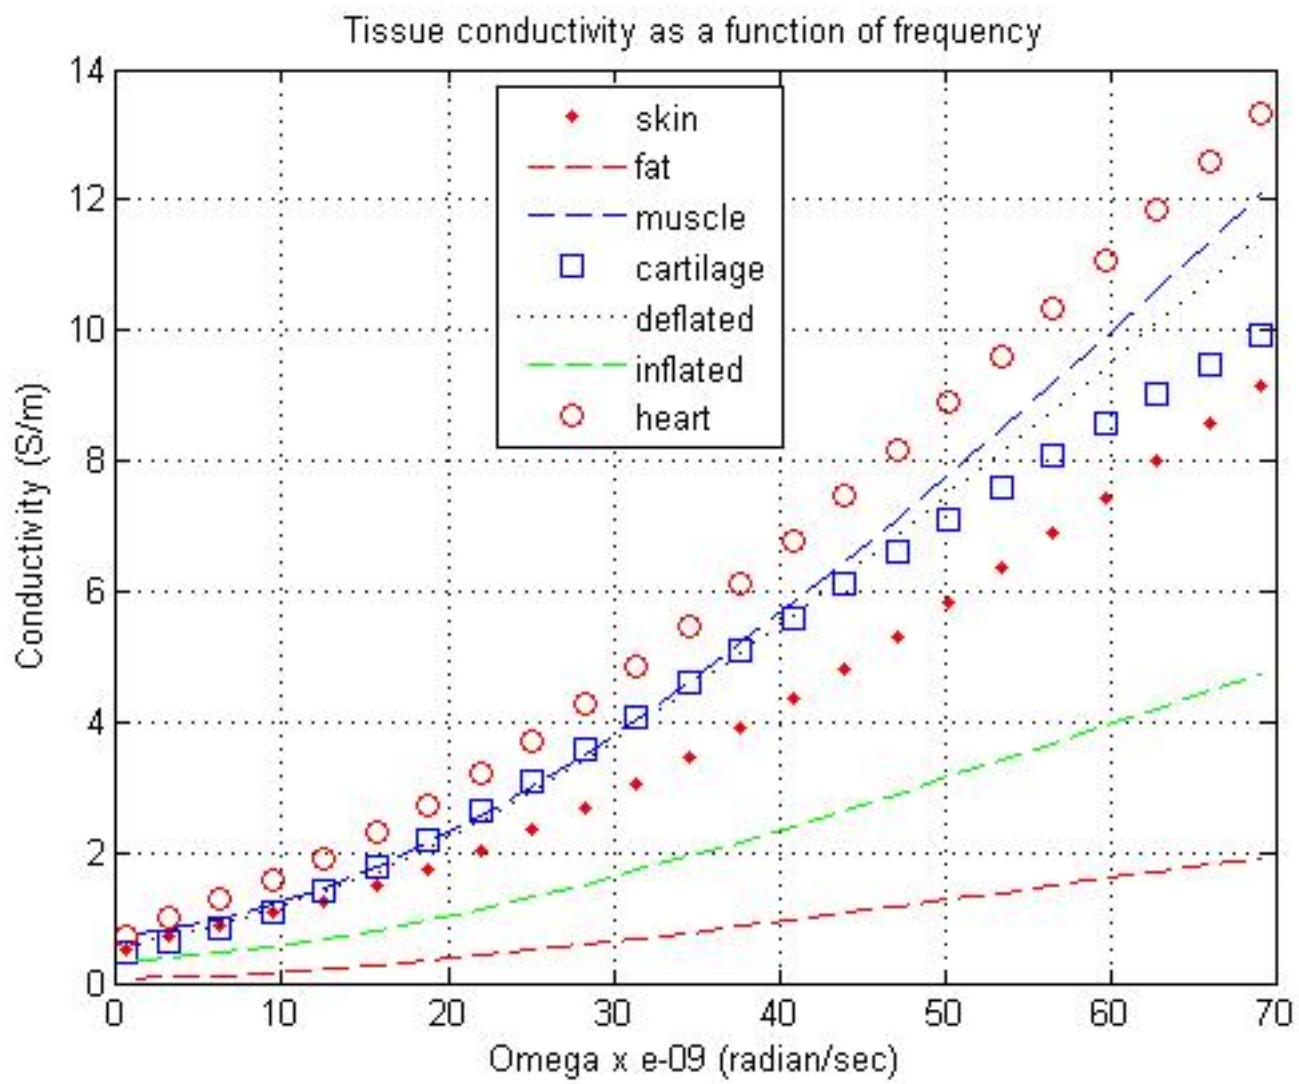

6

Figure 6: Figure 6 :



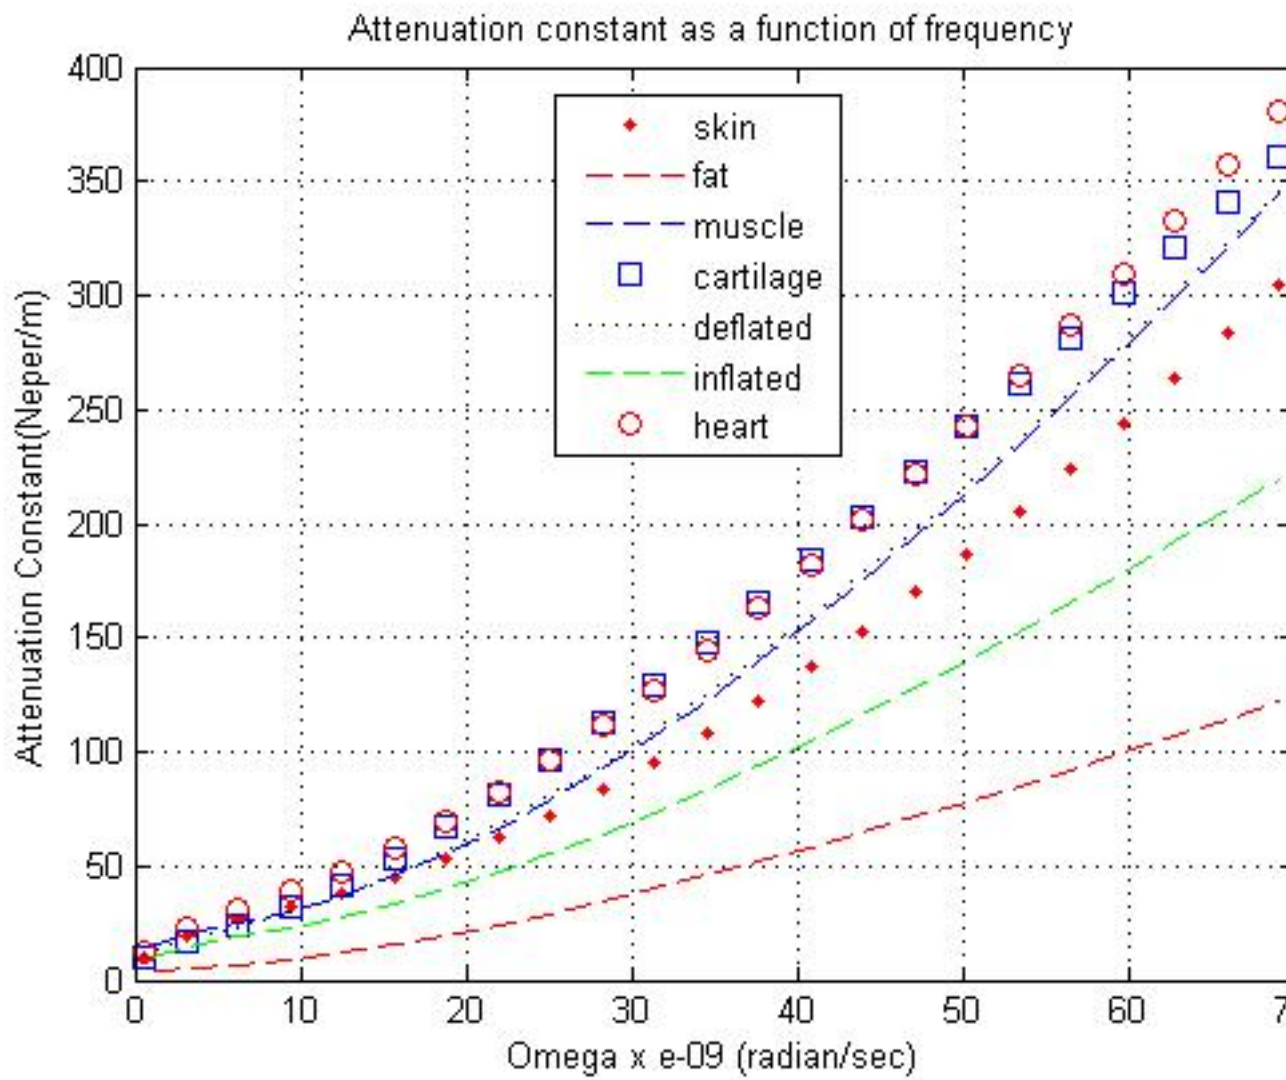

789

Figure 7: Figure 7 :Figure 8 :Figure 9 :

1

Tissue name	Thickness (mm)
Air	200
Skin(Dry)	1.5
Fat	9.6
Muscle	13.5
Cartilage	11.6
Lung	5.78

[Note: b) Frequency dependent dielectric properties of tissues in human thorax]

Figure 8: Table 1 :

I  
( ) F Volume XIV Issue III Version  
Global Journal of Researches in Engineering

Figure 9:

---

252 [ Global Journal of Researches in Engineering] , *Global Journal of Researches in Engineering*

253 [An internet resource for the calculation of the dielectric properties of body tissues] *An internet resource for the*

254 *calculation of the dielectric properties of body tissues*, Institute for Applied Physics, Italian National Research

255 Council

256 [An internet resource for the transverse section (2010)] *An internet resource for the transverse section*, <http://en.wikipedia.org/wiki/File:-Gray968.png> January 2010.

257

258 [Staderini ()] ‘An UWB radar based stealthy lie detector’. E M Staderini . *Ultra-Wideband, Short-Pulse*

259 *Electromagnetics 6*, E L Mokole, M Kragalott, K R Gerlach (ed.) (New York, USA) 2003. Kluwer Academic/

260 Plenum publishers. p. .

261 [Mcewan ()] ‘Body monitoring and imaging apparatus and method’. Thomas E Mcewan . *United States Patent*

262 1996. 5 p. 12.

263 [Mcewan ()] ‘Body monitoring and imaging apparatus and method’. Thomas E Mcewan . *United States Patent*

264 5, 1998. 766 p. 208.

265 [Franks et al. ()] ‘Contactless respiration monitoring of infants’. C I Franks , B H Brown , D M Johnston . *Med.*

266 *Biol. Eng* 1976. 14 (3) p. .

267 [Barber et al. ()] ‘Electromagnetic absorption in a multilayered model of man’. P W Barber , O P Gandhi , M

268 J Hagmann , Chatterjee , I . *IEEE T. Biomed. Eng* 1979. 26 (7) p. .

269 [Chirwa et al. ()] ‘Electromagnetic radiation from ingested sources in the human intestine between 150 MHz and

270 1.2 GHz’. L C Chirwa , P A Hammond , S Roy , D R S Cumming . *IEEE T Bio-med Eng* 2003. 50 p. .

271 [Martin et al. ()] ‘Frequency-dependent modeling of ultra-wideband pulses in human tissue for biomedical

272 applications’. O H Martin , G Martin , E Jones . *International Workshop on Ultra wide-band Systems Joint*

273 *with Conference on Ultra wide-band Systems and Technologies*, 2004. p. .

274 [Pisa et al. ()] ‘Monitoring of Cardio-pulmonary activity with UWB radar: A circuital model’. S Pisa , P Bernardi

275 , M Cavagnaro . *Asia-Pacific symposium on Electromagnetic Compatibility and 19 th International Zurich*

276 *Symposium on Electromagnetic Compatibility*, (Singapore) 2008.

277 [Gabriel ()] *Occupational and environmental health directorate, Radio frequency radiation division, Brooks Air*

278 *Force Base*, C Gabriel . N.AL/OE-TR-1996-0037. 1996. Texas, USA. (Compilation of the dielectric properties

279 of body tissues at RF and microwave frequencies)

280 [Chang ()] *The NPAC visible human viewer*, Y J Chang . 1997. New York. Syracuse University

281 [Staderini ()] ‘UWB radars in medicine’. E M Staderini . *IEEE Aerospace and Electronic System Magazine* 2002.

282 17 (1) p. .