Artificial Intelligence formulated this projection for compatibility purposes from the original article published at Global Journals. However, this technology is currently in beta. *Therefore, kindly ignore odd layouts, missed formulae, text, tables, or figures.*

SOFIA -Optical Operating System and Medical Analyses

Rafael Galli

3

1

2

Received: 14 December 2019 Accepted: 2 January 2020 Published: 15 January 2020

5 Abstract

⁶ Nursing is an area of extreme relevance to society. It is an area that requires intense

7 psychological due to excessive working hours. However, the accumulation of patients, added to

the exhaustion of the routine, causes many nurses to face psychological problems, such as the
Burnout syndrome. The assistance becomes impaired through a cascade effect. This set of
questions ends up generating a considerable delay in attendance, causing the hospital queues
to increase, which in turn causes an aggravation of the patients' diseases. The care of the

¹² elderly and children, especially children with down syndrome or autism, is more complicated

¹³ and, without attention, can make these people feel uncomfortable, stressed, or even enter into

- ¹⁴ a panic. The SOFIA project (Optical System of Operation and Medical Analysis) aims to
- ¹⁵ provide public hospitals and other similar places with an electronic system that can perform a
- ¹⁶ screening process more quickly, effectively, and non-invasively and monitoring the patients if
- 17 necessary.

18

41 **1** Introduction

 $_{\rm 42}~$ s reported in the media, the care of hospitals and health centers in Brazil has become increasingly precarious.

43 Said precariousness is due to the excessive workload, unhealthy conditions, and lack of PPE's; this affects the 44 psychological of the nurses, which can cause depression or Burnout syndrome, among other problems. All of this

⁴⁴ psychological of the habee, which can cause appression of Damoar Syndrom, among other prostenis. The other
 ⁴⁵ culminates in affecting patient care and the effectiveness of screening and monitoring. That said, the efficiency of

¹⁹ Index terms— effective, clinical exams, totem robot.

SOFIA -Optical Operating System and Medical is an area that requires intense psychological due to excessive 20 working hours. However, the accumulation of patients, added to the exhaustion of the routine, causes many 21 nurses to face psychological problems, such as the Burnout syndrome. The assistance becomes impaired through 22 a cascade effect. This set of questions ends up generating a considerable delay in attendance, causing the hospital 23 queues to increase, which in turn causes an aggravation of the patients' diseases. The care of the elderly and 24 25 children, especially children with down syndrome or autism, is more complicated and, without attention, can make these people feel uncomfortable, stressed, or even enter into a panic. The SOFIA project (Optical System 26 of Operation and Medical Analysis) aims to provide public hospitals and other similar places with an electronic 27 system that can perform a screening process more quickly, effectively, and non-invasively and monitoring the 28 patients if necessary. The device in question would sharply reduce nurses' workload, enabling them to perform 29 other tasks, given that they could only take care of hospitalized patients or those in serious condition, thus avoiding 30 the various problems mentioned above. The initial idea is for the construction of a totem robot that can travel 31 to the ill, performing an initial interaction with the person while, at the same time, acquiring the patient's data, 32 in addition to doing the screening process, being that initially, the robot would obtain the patient's temperature. 33 That said, a thermographic infrared sensor, which will measure the temperature on the foreheads of a person, 34 can fulfill this task. The active professional receives the data obtained at the end of the process. Also, to provide 35 a broader range of tests, such as glucose level exams, it is intended to add other sensors. All mechanisms are 36 controlled by a programmable microcomputer, which is very versatile for improvements and later changes in the 37 project. SOFIA has several advantages, such as the reduction of the professional's excessive workload, reducing 38 the cases of depression, or Burnout syndrome in them. It is worth noting this project's objective to help the 39 professionals, never to replace them. 40

46 care at health centers and similar places has become an increasingly relevant social problem in Brazil. Increasingly,

47 patients in public hospitals feel uncomfortable to perform examinations or for simple temperature monitoring;
48 also, we cannot ignore the nurse's health. Based on these facts, was developed the research project SOFIA -

49 Optical System of Operation and Medical Analysis; Which aims to optimize the acquisition of conventional clinical

50 examinations in the queues of hospitals and other similar places. The initial idea is the creation of an electronic

51 system capable of acquiring the temperature in a non-invasive way, ensuring a considerable optimization of the

52 medical service. The thermographic sensor would measure the patient's temperature and, through programmed 53 speech and voice communication, the robot would make a record for the patient; the professional would receive

53 speech and vo54 the sent data.

55 **2** II.

56 **3** Development

The first phase of the project's development aims to provide Brazilian hospitals and health centers with an 57 electronic device capable of quickly and noninvasively screening patients, acquiring the results of conventional 58 clinical examinations such as body temperature. The development of the project will take place in several stages. 59 In its first stage, the system would be able to capture a person's temperature through the forehead with the 60 thermographic sensor obtaining this data through a program on the microcomputer. This step, in turn, is 61 already partially completed; a calibration was performed but aimed at to do a more detailed one focused on 62 human applications. The new calibration process started, and; a small-scale prototype too. In the prototype, an 63 ultrasonic sensor and a voice recognition sensor would use together. The robot would use programmed speeches 64 to interact with the patient. The idea would be to make the device able to detect the distance of the patient 65 through the ultrasonic system and the programmed speeches. The robot would interact with the person asking 66 for his data; In turn, the voice recognition device would capture everything the patient says and then set up their 67 profile with the results of the screening; The doctor at the end of the process would receive these profiles via wifi. 68 It is to add new sensors to perform other types of tests, in particular, the glucose test. The device would use 69 the infrared to capture the level of sugar in the blood, so it would not be necessary to pierce the finger as is the 70 conventional examination. The advantage of being done this way is that it is non-invasive; it would make people 71 do it more often since many do not like the conventional way. This step would be developed based on the thesis 72 "Glucose monitoring system in a continuous and noninvasive way to the human body based on spectroscopy and 73 photoplethysmography methods" (Santos, Samuel, 2017). The aim is also to be able to use the thermographic 74 image to perform the breast cancer exam; in this way, it would be non-invasive. 75

$_{76}$ 4 a) The micro-computer

The Raspberry pi 3 B plus (Figure 1), produced by the Raspberry Pi Foundation, is a micro-computer that uses 77 the Broadcom BCM2837B0 processor, which is very versatile and intuitive. The microcomputer acquires the 78 sensor data, sending this information to the professional. This development board selected for its high processing 79 capacity and the ease of implementation of other sensors. The temperature sensor chosen was the AMG8833 80 (Figure 2); Panasonic Industries produced the device; however, the plate printed by Adafruit Industries, the same 81 82 as a thermographic device, ends up capturing the temperature in the form of an image. The AMG8833 has an 83 accuracy of + -2.5°C but can circumvent through calibration. It also uses the I2C interface, which facilitates the connection with the microcomputer. The minimum temperature for use would be 0° C and the maximum 80° C; 84 it is also sensitive to humidity, operating at 15% to 85% R.H. Outside this range, it can end up deteriorating. 85 The capture of the sensor can see it in Figure 3, where it shows the operation. It's worth point out that the 86 acquisition distance also influences the reading, being that it measures up to 7m, however in practice, to measure 87 a person, the maximum is + -30cm. The device itself works as a matrix; that is, if you capture the image 88 of a specific point that is capable of measuring the human body, such as the forehead and the armpit when 89 averaging that matrix, you find the temperature in common. That said, it was necessary to perform a calibration 90 to make sure that the average is indeed correct. For this, were used a Peltier plate, a bench power supply, a 91 multimeter, and a thermocouple. With the source, it was possible to control the temperature of the Peltier plate; 92 93 the thermocouple would be the base temperature sensor. In this way, were recorded in an excel spreadsheet the 94 values that the thermocouple and the sensor captured. Also, were noted the day temperature, humidity, current, 95 and voltage, as seen in Figure 4; However, this was only for academic purposes; Since what matters in the graph 96 is the thermocouple and sensor data. The thermocouple was X, and the sensor was Y, as can be seen in Figure ?? Figure ??: Graph of the temperature between the thermocouple and the sensor In the sensor program to 97 correct the errors of the amg8833, was placed the equation (??). 98

(1) However, it was an initial test; to correct all errors will be done a more detailed one. To not invade the patient's personal space, the equipment will have characteristics that can provide this requirement; and will be designed with materials that cannot damage the skin or cause any allergy or any other unforeseen to the patient.

¹⁰² 5 c) Set Sensor-Microprocessor

The connection sensor-microprocessor is an I2C connection, as shown in Figure 6, so the red wire connects the 103 raspberry's 3V3 pin to the VIN pin of the sensor; yellow connects the two SDAs; blue connects the two SCLs; and 104 finally, black connects the two GNDs. The basic program, available on the Adafruit Industries website (Rembor, 105 Kattini, 2019), was posteriorly downloaded. Is not calibrated the initial code, than was necessary a calibration. 106 After these processes, was placed in the program, the equation (??). With a thermographic sensor, it is possible 107 to capture the body structure at the temperature, as in Figure 7. The idea would be to use it to detect other 108 problems, being possible even to detect breast cancer. To obtain the right distance for an ideal temperature 109 reading will be used as an ultrasonic sensor, the model HC-SR04 (Figure 8); The sensor works with distances 110 from two centimeters to four meters. The idea is to use prepared speeches where it will tell if the patient should 111 move away or get closer, to leave him where the sensor can measure the temperature correctly. 112

¹¹³ 6 e) Prototype

As stated earlier, the intention is to create a small-scale prototype; the idea is to create a totem robot. The project already has a prototype design (Figure 9). The design was made especially for this project; the robot's face would consist of a small LCD screen that connects to the raspberry, the sensor would be in the lower right corner.

118 **7 III.**

¹¹⁹ 8 Results and Discussions

Currently is partially completed the calibration process for the AMG-8833 thermographic sensor. The device 120 already works with the initial calibration; however, to achieve greater precision and superior quality in 121 122 temperature acquisitions, a more detailed calibration will be performed. The project presented at technological exhibitions and the result of the temperature measurements with the initial calibration is entirely satisfactory. 123 To analyze the approval of the project will be carried out a popular survey. Will interviewed health professionals 124 to obtain an approval index about the possible effectiveness of the prototype in the field, possible implementation 125 in health establishments in Brazil, and widespread approval regarding the willingness to undergo robot analysis. 126 IV. 127

¹²⁸ 9 Conclusions and Future Works

The project has many health benefits; As mentioned before, it could decrease the nurse's workload, thus reducing 129 cases of exhaustion that lead to depression or burnout syndrome, in addition to improving care, making it 130 faster and not invasive. There are still some issues, more accurate calibration, and the prototype test in the 131 field. Despite this, it already shows great potential; Since, with the initial calibration, it was already able to 132 measure people's temperature correctly. It is estimated to create an interactive interface in conjunction with 133 the programmed speeches; this would facilitate the user's interaction with the robot. After the exchange, as 134 previously mentioned, the active professional would receive the obtained data professional. It is intended in the 135 future to add other sensors to expand the range of exams. In principle would be created a sensor to measure 136 glucose based on infrared, as it would be non-invasive without the need to pierce the finger. The idea for the 137 construction of this device is based on the "Glucose monitoring system in a continuous and non-invasive way to 138 the human body based on spectroscopy and photoplethysmography methods" (Santos, Samuel, 2017). Also, the 139 possibility of obtaining another thermographic sensor more powerful, it is being studied. Still, of low cost, the 140 idea will be to use it to perform the examination of breast cancer in a non-invasive way. 141

 $^{^{1}}$ © 2020 Global Journals



Figure 1: Figure 1 :

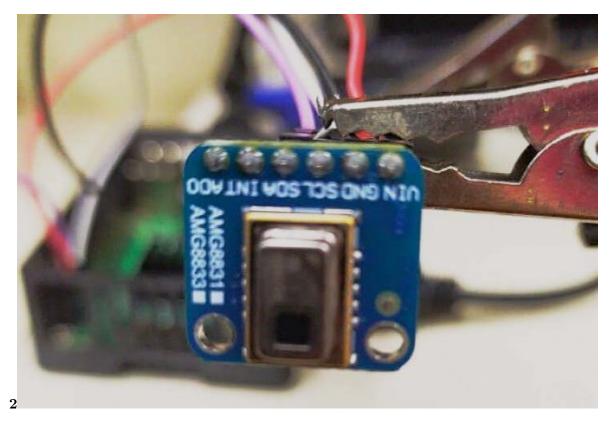


Figure 2: Figure 2 :


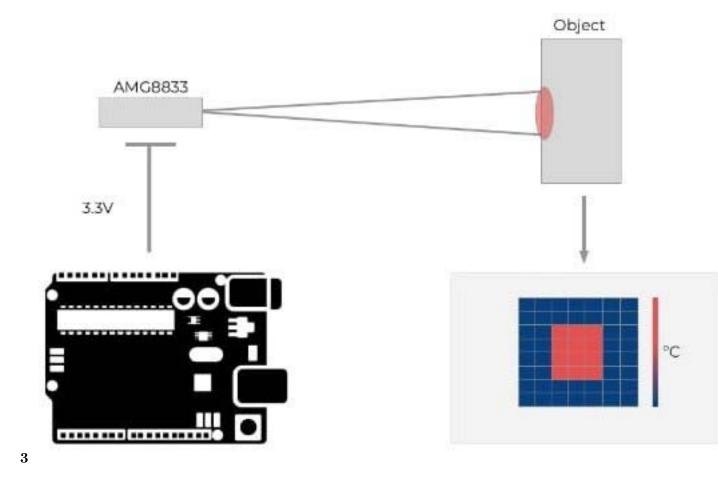


Figure 3: Figure 3 :

TEMP	MOISTURE		
26°C	68%		
CURRENT	VOLTAGE	THERMOCOUPLE	SENSOR
0	0	28	2,4
0,05	0,2	29	31
0,1	0,4	29	23,567
0,15	0,5	30	3,85
0,2	0,8	31	24,733
0,25	0,8	33	26,367
0,3	1,2	34	27,3
0,35	1,3	36	29,9
0,4	1,5	38	31,5
0,45	1,7	40	32,433
0,5	2	43	34,717
0,55	2,2	46	35,7

 $\mathbf{4}$

Figure 4: Figure 4 :

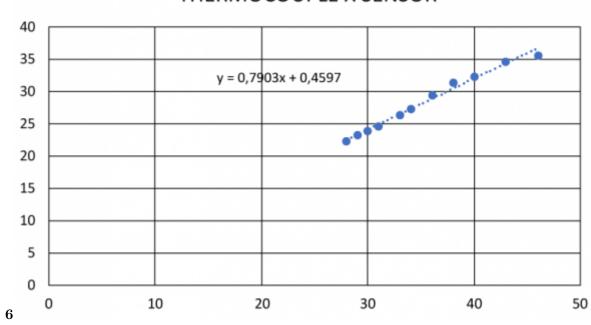

THERMOCOUPLE X SENSOR

Figure 5: Figure 6 :

$$_{7}$$
 Y = 0,7903x -0,4597

Figure 6: Figure 7 :

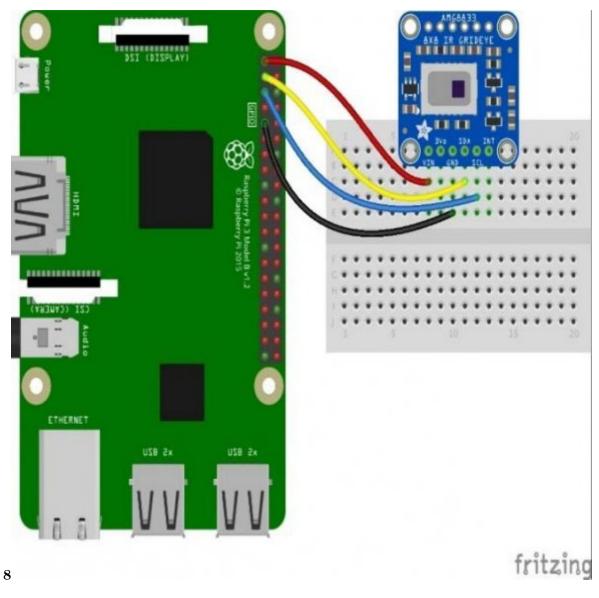


Figure 7: Figure 8 :



Figure 8: Figure 9 :

- 142 [Articles] , Articles .
- 143 [Tsai and Shang-Ru] , Tsai , Shang-Ru .
- [Hamblin ()] Biological Effects and Medical Applications of Infrared Radiation: 170, Michael R Hamblin . 2017.
 Elsevier.
- [Vatansever et al. ()] Far Infrared Radiation (FIR): Its Biological Effects and Medical Applications: 1, Fatma ;
 Vatansever , Hamblin , R Michael . 2012. De Gruyter.
- [Markenhof ()] 'Integrating a Temperature Sensor into a CMOS Image Sensor, 2015, 56f. Dissertação Mestrado'.
 J Markenhof . *Holanda* 2015. Universidade Técnica de Delft
- 150 [Mandel et al. ()] Low-Level Laser Therapy: 1, Arkady ; Mandel , Hamblin , R Michael . 2012. De Gruyter.
- 151 [Rembor ()] Python & CircuitPython, Kattini Rembor . <https://learn.adafruit.com/
 adafruit-amg8833-8x8-thermal-camera-sensor/python-circuitpython> 2019. (Acesso em 13
 153 de março)
- [References Références Referencias Monographs, dissertations, and theses] References Références Références Referencias
 Monographs, dissertations, and theses,
- 156 [Santos ()] 'Sistema de monitoração de glicose de modo continuo e não invasivo ao corpo humano baseados
- em métodos de espectroscopia e fotopletismografia, 2017, 96f. Trabalho de Conclusão (Graduação)'. Samuel
 Santos . Instituto Federal Sul Rio Grandense (IFSUL) 2017.